

AUSTENAL

JUL 31 2000

R001798

4101 W. 51ST STREET
CHICAGO, IL 60632-4287
TEL 773.735.0600
800.621.0381
FAX 773.735.3940

**Unalloyed Titanium for the DCS Precident CAD/CAM System
510(k) Premarket Notification Summary**

The Unalloyed Titanium for the DCS CAD/CAM System is furnished in a block form that is designed for use as the feed stock for the DCS Precident CAD/CAM System to produce copings and/or substrates for fixed dental restorations; i.e. porcelain fused to metal restorations.

Unalloyed Titanium has been in use successfully as part of the DCS Precident System in Europe and a predicate product exists on the US Market.

The safety and efficacy of Unalloyed Titanium is well established. This material complies with the requirements of ASTM F 67-95 Standard Specification for the Unalloyed Titanium for Surgical Implant Applications. The suitability of Unalloyed Titanium for the substructure of dental restorations has also been demonstrated in the dental industry in predicate CAD/CAM Systems.



DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

JUL 31 2000

Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

Mr. Ronald Dudek
Director of Technical Resources
Austenal Incorporated
4101 West 51st Street
Chicago, Illinois 60632-4287

Re: K001798
Trade Name: DC Titan
Regulatory Class: II
Product Code: EJH
Dated: June 7, 2000
Received: June 14, 2000

Dear Mr. Dudek:

We have reviewed your Section 510(k) notification of intent to market the device referenced above and we have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.


If your device is classified (see above) into either class II (Special Controls) or class III (Premarket Approval), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 895. A substantially equivalent determination assumes compliance with the Current Good Manufacturing Practice requirements, as set forth in the Quality System Regulation (QS) for Medical Devices: General regulation (21 CFR Part 820) and that, through periodic QS inspections, the Food and Drug Administration (FDA) will verify such assumptions. Failure to comply with the GMP regulation may result in regulatory action. In addition, FDA may publish further announcements concerning your device in the Federal Register. Please note: this response to your premarket notification submission does not affect any obligation you might have under sections 531 through 542 of the Act for devices under the Electronic Product Radiation Control provisions, or other Federal laws or regulations.

Page 2 - Mr. Dudek

This letter will allow you to begin marketing your device as described in your 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4692. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21CFR 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its internet address "<http://www.fda.gov/cdrh/dsma/dsmamain.html>".

Sincerely yours,

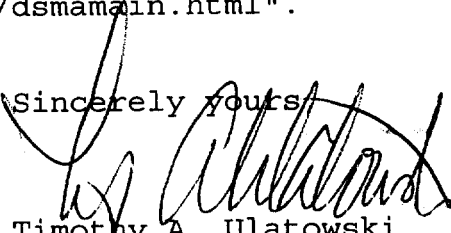

Timothy A. Ulatowski
Director

Division of Dental, Infection Control
and General Hospital Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure

510(k) Number (if known): K001798

Device Name: DC-TITAN

Indications For Use:

DC-TITAN is intended for use in the fabrication (via CAD/CAM techniques) of the metal substructure of porcelain fused to metal fixed dental restorations; namely crowns and bridges.

(PLEASE DO NOT WRITE BELOW THIS LINE-CONTINUE ON ANOTHER PAGE IF NEEDED)

Concurrence of CDRH, Office of Device Evaluation (ODE)



(Division Sign-Off)

Division of Dental, Infection Control,
and General Hospital Devices

510(k) Number K001798

Prescription Use ☒
(Per 21 CFR 801.109)

OR

Over-The-Counter Use ☐

(Optional Format 1-2-96)